

Sample Received: June 30, 2026

COA Issued: July 6, 2026

PRODUCT INFORMATION

Vendor: NexAmino Sample Name: KLOW 80mg Sample Type: Blue lyophilized powder Lot Number: NA MW (g/mol): 403.2, 342.4, 889.1, 1419.5

ANALYTICAL METHODS

Identity: Confirmed via LC-MS/MS



Purity: RP-HPLC (214 nm)

Content: HPLC quantitation

TEST RESULTS

Specification	Result	Method	Status
Identity: KLOW	GHK-Cu, KPV, TB-500, BPC-157	MALDI-MS	✓ Conforms
Content	50.26, 10.66, 10.94, 10.24 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.9%	RP-HPLC (214 nm)	✓ Conforms

HPLC Chromatogram (Retention Time: 1.979, 2.109, 2.315, 9.159 min)

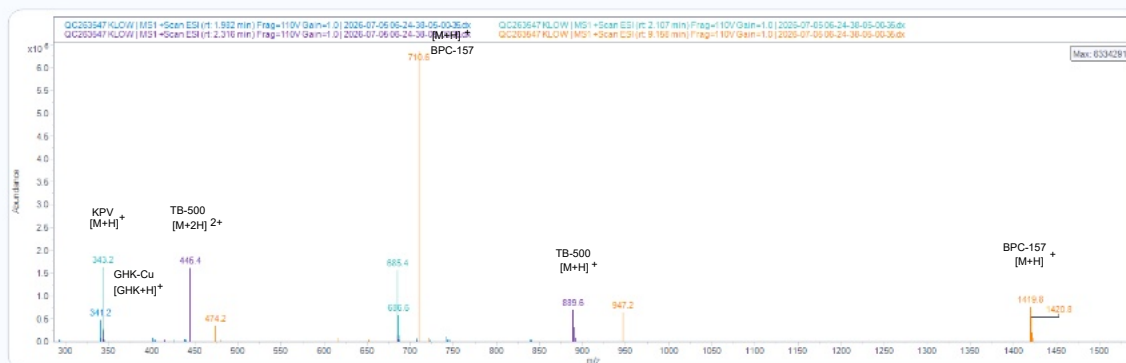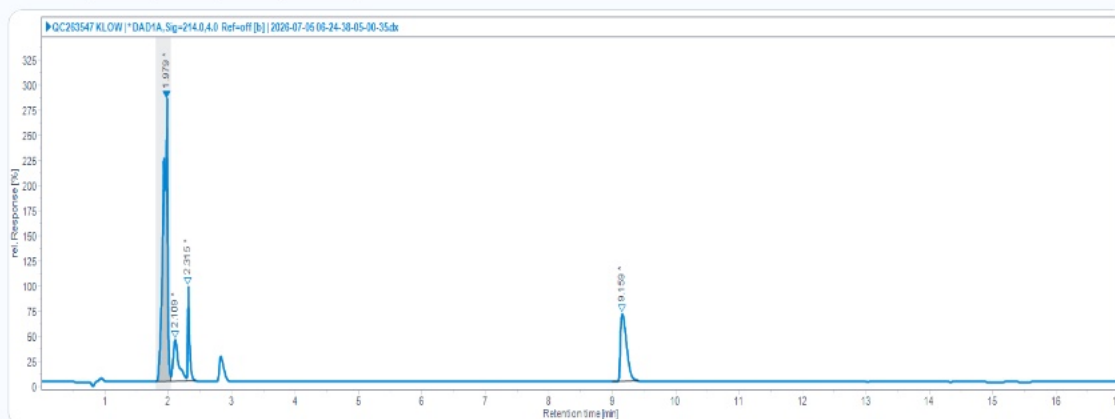

Certification: This COA confirms that the tested material meets or exceeds Bioviridian's analytical quality specifications for peptide research use.

Visit: <https://bioviridians.com/coa-search.html>*Shane Straight*Shane Straight, M.S.
Principal Chemist, Bioviridian Inc.